COPYCETV CHECT




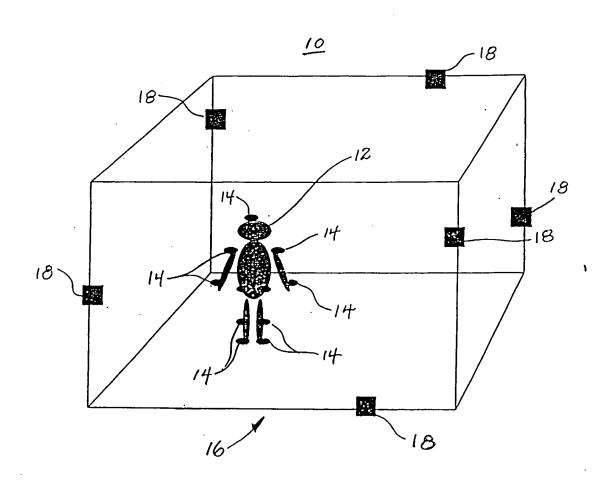


Fig. 1

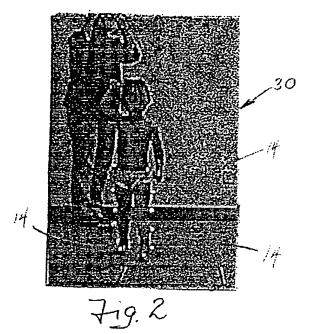

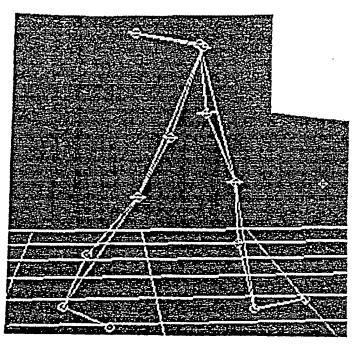



719.3

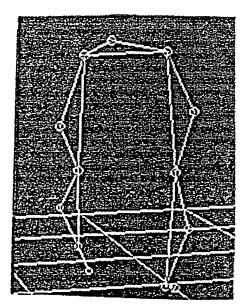

719.4

EST AVAILABLE COPY 23 25 INDUSTRY 5mm PERFORMANCE IMPROVEMENT ACCURACY 26 ANIMATION /mm CLINICAL Omm HOURS DAYS REAL TIME MINUTES 22 PROCESSING TIME

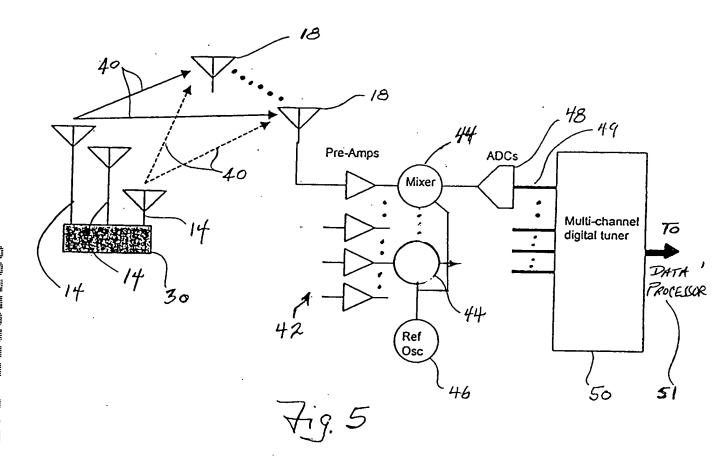

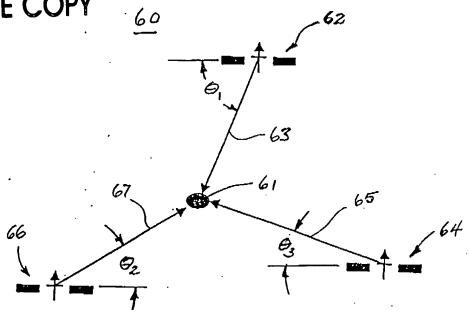



PRIOR ART

rosero, kedoka

Fig.6



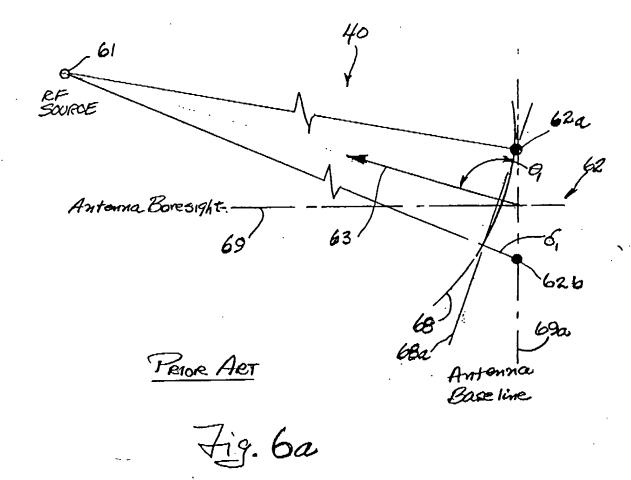

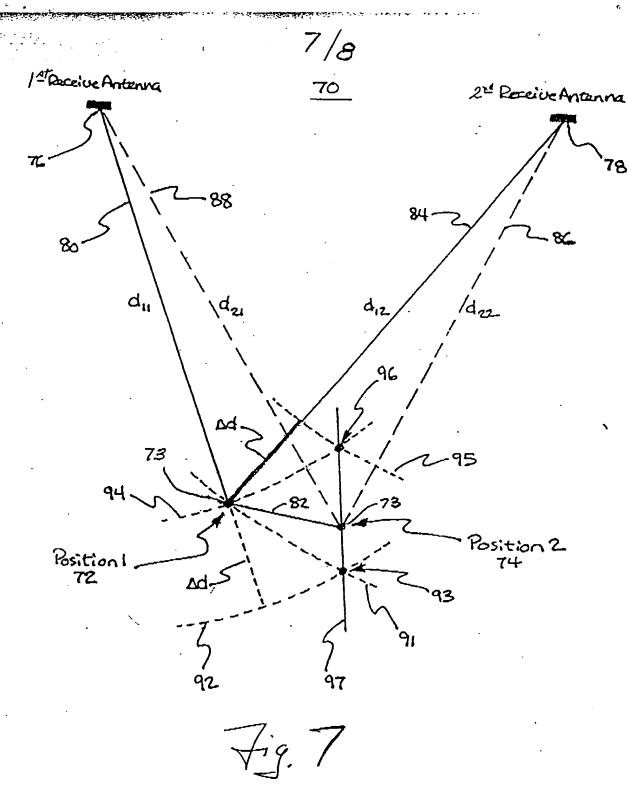



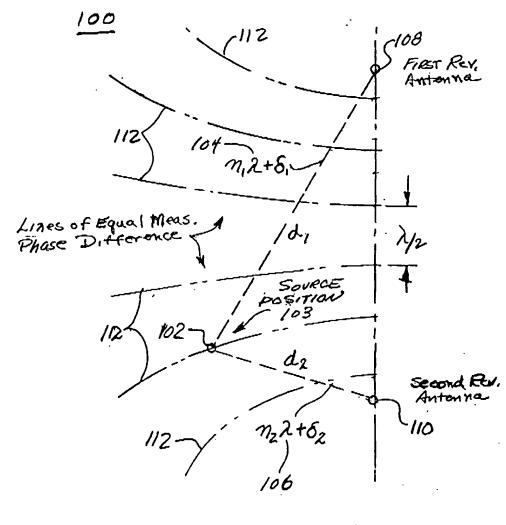


Fig. 8